

Rigid Ring for Valve Annuloplasty - Braile



Experience
Quality
Performance

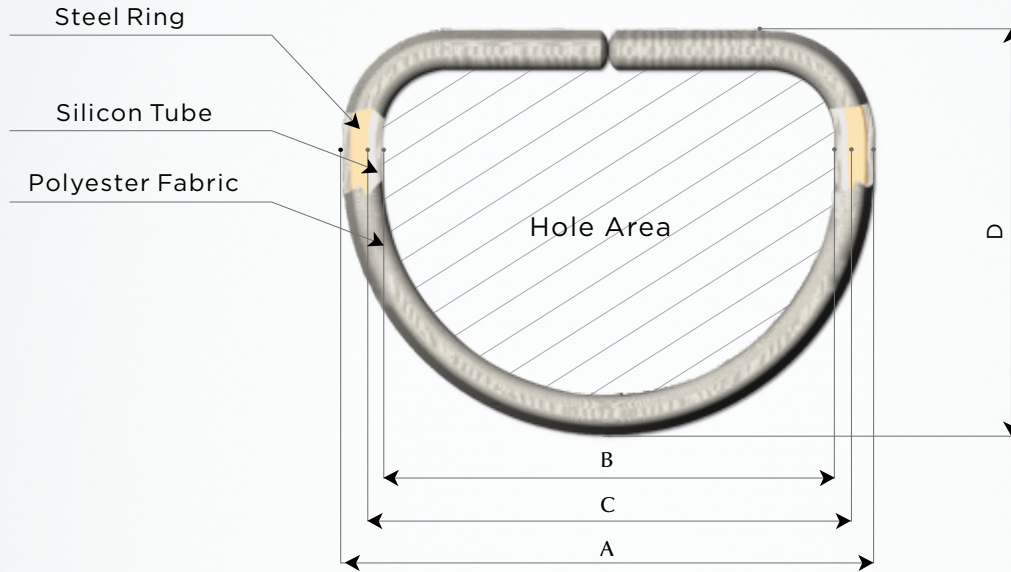
 **BRAILE**[®]
BIOMÉDICA

Description:

The Rigid Ring for Valve Annuloplasty - Braile is made of stain less steel and recovered by a silicon tube and coated with polyester.

Indication:

The Rigid Ring for Valve Annuloplasty - Braile is used for Mitral valve repair in reconstructive surgery of Mitral valve, whose purpose is to put the retracted mitral valve in its anatomic natural position, remodel the distended commissures and correct the Mitral ring dilatation, distributing the traction forces by means of wrinkling.

**TECHNICAL SPECIFICATIONS**

Size	A(mm) ± 0,5	B(mm) ± 0,5	C(mm) ± 0,5	D(mm) ± 0,5	Hole Area (cm) ± 20	Code
24	28,3	23,1	24	21,2	308	2088
26	30,3	25,1	26	23,2	379	2091
28	32,3	27,1	28	25,2	456	2103
30	34,3	29,1	30	27,2	539	2116
32	36,3	31,1	32	29,2	629	2129
34	38,3	33,1	34	31,2	725	2132
36	40,3	35,1	36	33,2	826	2145
38	42,3	37,1	38	35,2	938	202915